
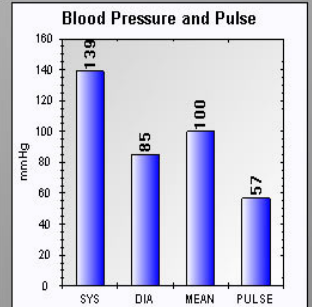
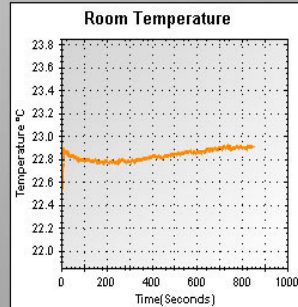
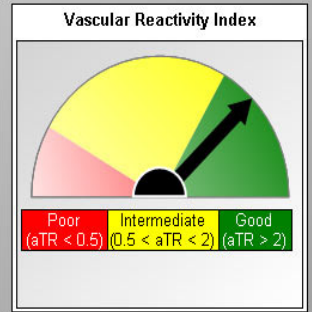
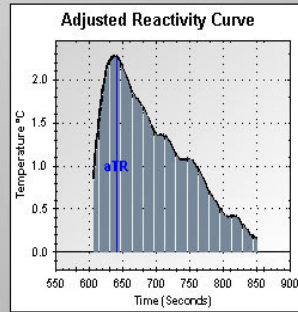


VENGuard V19

— Right Finger (R) — Left Finger (L) — Zero Reactivity Curve (ZRC)
····· (R - L) — (R-ZRC) — Room Temperature

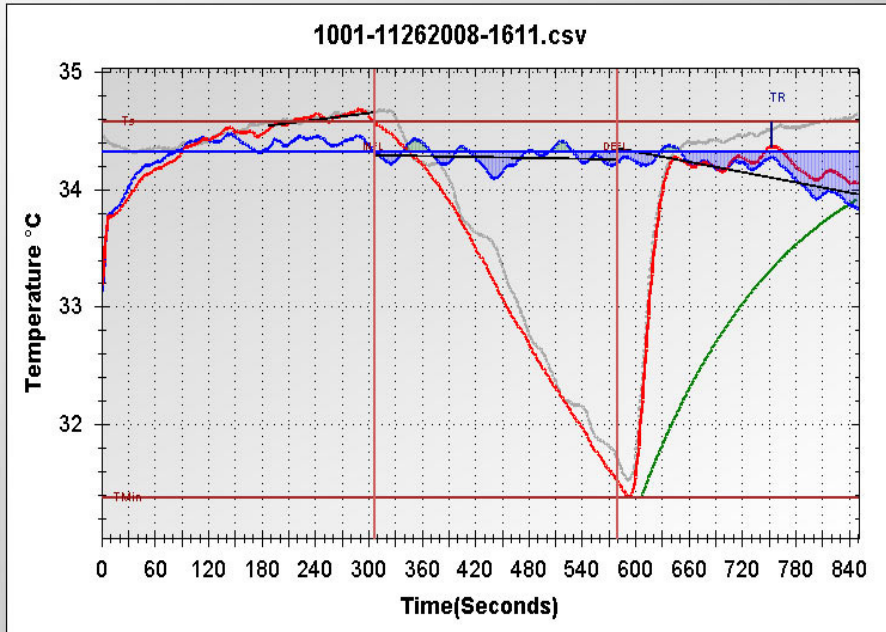

Flags:

- Cold Finger
- Sympathetic Response
- Stabilization
- Finger Room Delta
- Cold Room
- Fluctuating Room Temp
- Right vs Left

VENDYS Indices:

TR: -0.28
 TMP-AUC: 453.3
 aTMP-AUC: 281.51
 NVR Inflation: 0.08
 NVR Deflation: 0
 Room Temperature: 22.85
 Sympathetic Code:

Vascular Reactivity Index
aTR = 2.26

Endothelix
 Date/Time of Test
 11/26/2008 10:03:47 AM